

# Characterization of 10 cutaneous tumors with ex vivo LC-OCT: A novel tool in dermato-oncological surgery with margin control?

Pau Rosés Gibert<sup>1</sup>, Jean-Luc Perrot<sup>2</sup>, Kassandra Groux<sup>3</sup>, Jonas Ogien<sup>3</sup>, Javiera Pérez-Anker<sup>1</sup>, Josep Malvehy<sup>1</sup>

<sup>1</sup>Dermatology department, Hospital Clínic de Barcelona; <sup>2</sup>Dermatology department, Centre Hospitalier Universitaire de Saint Étienne; <sup>3</sup>DAMAE Medical, Paris

## INTRODUCTION

Currently, we have numerous imaging techniques for skin evaluation, such as in vivo and ex vivo reflectance confocal microscopy (RCM), optical coherence tomography (OCT), and Linefield Confocal OCT (LC-OCT). With LC-OCT technology, a vertical image similar to histology, a horizontal image similar to RCM, and a three-dimensional image can be obtained. A new prototype that allows obtaining ex vivo images with LC-OCT has been developed. This not only facilitates a more comprehensive understanding of the histology of cutaneous tumors but also holds promise for advancing surgical margin detection in the future.


## OBJECTIVES

The aim of this project is to evaluate the quality of images obtained with ex vivo LC-OCT in different cutaneous tumors, describe the morphological characteristics of the evaluated lesions and correlate them with dermoscopy, in vivo RCM, in vivo LC-OCT and histology.

## METHODOLOGY


We prospectively evaluated patients with diverse cutaneous tumors between June 2022 and July 2023, with the following inclusion criteria: 18 years and a cutaneous tumor on the trunk and limbs. We collected clinical, dermoscopic, RCM, in vivo LC-OCT, ex vivo LC-OCT (Fig 1.), and histopathological images of different types of cutaneous tumors.

**Fig. 1:** Description of the ex vivo LC-OCT system and its modularity (a) Design of the platform (b) Design of the sample-holder and the positioning of the sample in it (cross-section view) (c) Top view of the sample-holder containing a sample, a visualisation of the mosaic process is shown (d) 2D horizontal mosaic imaging pattern (e) 3D mosaic imaging pattern. FOV: Field-of-view. Axes: representing the movement of the XY motorized stage.

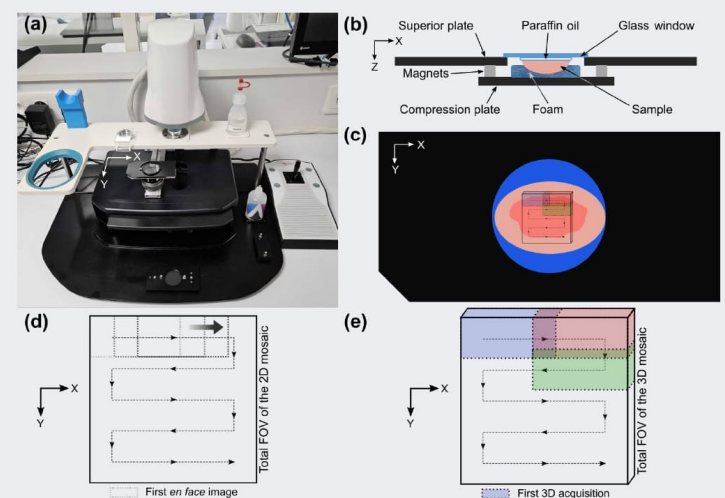


## RESULTS AND CONCLUSIONS


In total, 10 cutaneous tumours from 10 patients were evaluated using this new technology: 3 melanomas, 2 seborrheic keratoses, 2 basal cell carcinomas, and 3 melanocytic nevi. For the first time, we have been able to visualize excised cutaneous tumors in three dimensions. The images obtained are equivalent to those acquired with in vivo devices. We have appreciated cellular resolution and conducted cellular correlation with confocal microscopy, in vivo LC-OCT, and histology (Figs 2-4). These promising results may initiate further investigations into the assessment of this technology in dermato-oncological surgery with margin control.

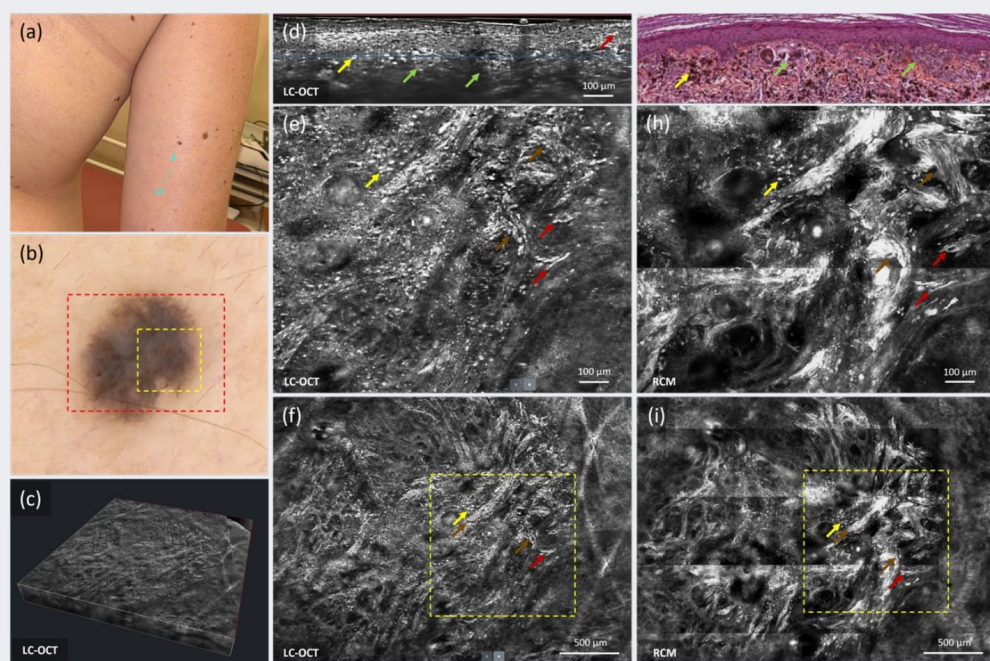

**Figure 2. A)** Clinical image of a brown-black macule. **B)** Dermoscopy image showing blue and black structureless areas, pigmented parakeratosis and atypical network pattern at the periphery. **C)** LC-OCT ex vivo 3D mosaic. **D)** LC-OCT ex vivo vertical view: Atypical melanocytes (red arrow), disrupted DEJ, atypical nests (green arrow) and melanophages (yellow arrows). **E)** LC-OCT ex vivo horizontal view: Atypical meshwork pattern (brown arrows) with thickening junctions, inflammatory cells (yellow arrow) and atypical dendritic cells (red arrows). It is noticeable that cell details are less saturated compared to RCM in H image. **F)** LC-OCT ex vivo: Atypical meshwork pattern (brown arrows) with thickening junctions, inflammatory cells (yellow arrow) and atypical dendritic cells (red arrows). **G)** Histology image: Disrupted DEJ, abundant melanophages and inflammatory cells (yellow arrows) and atypical melanocytic nests (green arrow). **H)** RCM ex vivo image: Atypical meshwork pattern (brown arrow) with thickening junctions, inflammatory cells (yellow arrow) and atypical dendritic cells (red arrows). It is noticeable that cell details are saturated compared to LC-OCT ex vivo image E. **I)** RCM ex vivo image: Atypical meshwork pattern (brown arrow) with thickening junctions, inflammatory cells (yellow arrow) and atypical dendritic cells (red arrows).

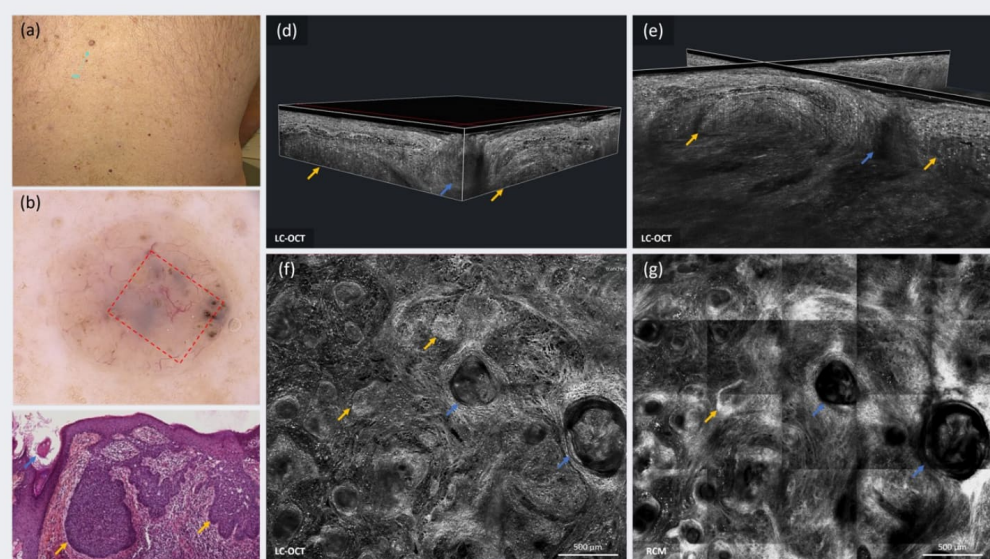

**Figure 3. A)** Clinical image of a pink-brownish papule. **B)** Dermoscopy: arborizing vessels, pseudocysts, blue-grey ovoid nests and spoke-wheel structures. **C)** Histology image: Basal cell carcinoma lobules (orange arrows) with palisading and a keratin plug (blue arrow) can be observed. **D)** LC-OCT ex vivo 3D mosaic. **E)** LC-OCT ex vivo vertical view: BCC lobules (orange arrow) and keratin plugs can be seen (blue arrow). **F)** ex vivo RCM: hyporefractile lobules (orange arrows), hyporefractile cysts, clefting and keratin plugs (blue arrows). **G)** ex vivo LC-OCT: hyporefractile lobules (orange arrow), hyporefractile cysts, clefting and keratin plugs (blue arrows)

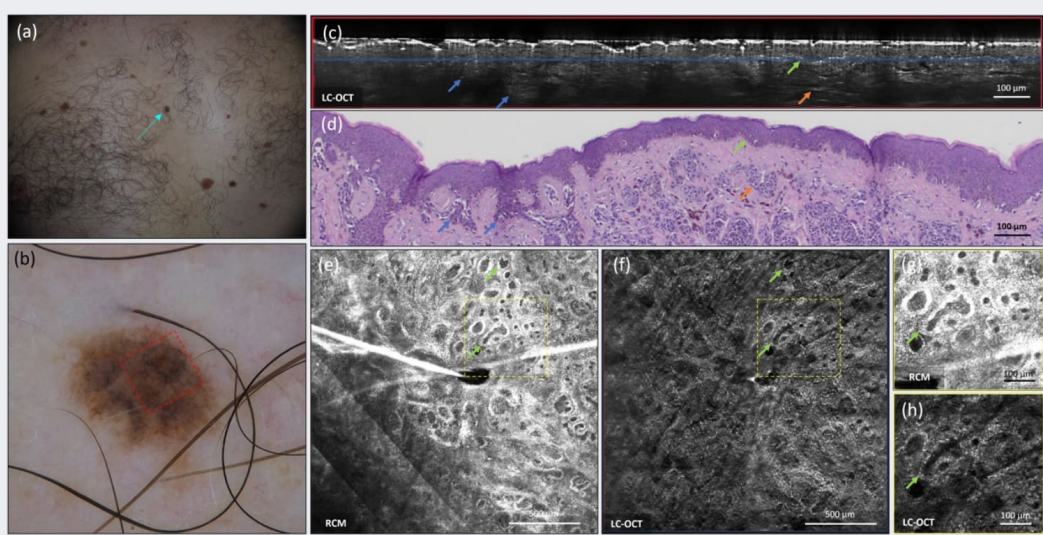

**Figure 4. A)** Clinical image. **B)** Dermoscopy: Atypical brown network pattern and loss of central structures. **C)** LC-OCT ex vivo vertical view: Lentiginous melanocytic proliferation with a pigmented basal layer (green arrows), junctional nests of melanocytes (blue arrows) and wave-like pattern that corresponds to collagen fibers around hypopigmented nests (orange arrows). **D)** Histology image: Lentiginous melanocytic proliferation with a pigmented basal layer (green arrows), junctional nests of melanocytes (blue arrows) and hypopigmented nests (orange arrows). **E)** In vivo RCM horizontal view: Ringed pattern (green arrows). **F)** Ex vivo LC-OCT horizontal view: Ringed pattern (green arrows). **G)** In vivo RCM: ringed pattern detail (green arrow). **H)** LC-OCT ex vivo Ringed pattern detail (green arrow).

## REFERENCES

1. Simões MCF, Sousa JJS, Pais AAC. Skin cancer and new treatment perspectives: A review. *Cancer Lett.* 2015;357(1):8–42.
2. Soglia S, Pérez-Anker J, Lobos Guede N, Glavedoni P, Puig S, Malvehy J. Diagnostics Using Non-Invasive Technologies in Dermatology. *Cancers (Basel).* 2022;14(23).
3. Schuh S, Rulnic C, Sattler E, Welzel J. Confocal line-field OCT. *Hautarzt.* 2021;72(12):1039–47.
4. Dubois A, Levesq O, Azimani H, Siret D, Barut A, Suppa M, et al. Line-field confocal optical coherence tomography for high-resolution noninvasive imaging of skin tumors. *J Biomed Opt.* 2018; Oct 23;23(10):1.
5. Tannous ZS, Mihm MC, Flotte TJ, González S. In vivo examination of lentigo maligna and malignant melanoma in situ, lentigo maligna type by near-infrared reflectance confocal microscopy: Comparison of in vivo confocal images with histologic sections. *J Am Acad Dermatol.* 2002;46(2):260–3.
6. González S, Rajadhyaksha M, Rubinstein G AR. Characterization of psoriasis in vivo by reflectance confocal microscopy. *J Med.* 1999;30(5-6):337–56.
7. Malvehy J, Pérez-Anker J, Toll A, Pigem R, Garcia A, Alos LL, et al. Ex vivo confocal microscopy: revolution in fast pathology in dermatology. *Br J Dermatol.* 2020;183(6):1011–25.
8. Pérez-Anker J, Malvehy J, Moreno-Ramírez D. Ex Vivo Confocal Microscopy Using Fusion Mode and Digital Staining: Changing Paradigms in Histological Diagnosis. *Actas Dermo-Sifiligráficas (English Ed.* 2020;111(9):236–42.
9. Guerrero JA, Pérez-Anker J, Fernández-Esparrach G, Archilla I, Diaz A, Lopez-Prades S, et al. Ex vivo Fusion Confocal Microscopy of Colorectal Polyps: A Fast Turnaround Time of Pathological Diagnosis. *Pathobiology.* 2021;88(6):392–9.
10. Wan B, Ganier C, Du-Harpru X, Harun N, Watt FM, Patalay R, et al. Applications and future directions for optical coherence tomography in dermatology\*. *Br J Dermatol.* 2021;184(6):1014–22.